

PROCEEDINGS OF SPIE

Remote Sensing System Engineering

**Philip E. Ardanuy
Jeffery J. Puschell**
Editors

**11–13 August 2008
San Diego, California, USA**

Sponsored and Published by
SPIE

Volume 7087

Proceedings of SPIE, 0277-786X, v. 7087

SPIE is an international society advancing an interdisciplinary approach to the science and application of light.

The papers included in this volume were part of the technical conference cited on the cover and title page. Papers were selected and subject to review by the editors and conference program committee. Some conference presentations may not be available for publication. The papers published in these proceedings reflect the work and thoughts of the authors and are published herein as submitted. The publisher is not responsible for the validity of the information or for any outcomes resulting from reliance thereon.

Please use the following format to cite material from this book:

Author(s), "Title of Paper," in *Remote Sensing System Engineering*, edited by Philip E. Ardanuy, Jeffery J. Puschell, Proceedings of SPIE Vol. 7087 (SPIE, Bellingham, WA, 2008) Article CID Number.

ISSN 0277-786X
ISBN 9780819473073

Published by

SPIE

P.O. Box 10, Bellingham, Washington 98227-0010 USA
Telephone +1 360 676 3290 (Pacific Time) · Fax +1 360 647 1445
SPIE.org

Copyright © 2008, Society of Photo-Optical Instrumentation Engineers

Copying of material in this book for internal or personal use, or for the internal or personal use of specific clients, beyond the fair use provisions granted by the U.S. Copyright Law is authorized by SPIE subject to payment of copying fees. The Transactional Reporting Service base fee for this volume is \$18.00 per article (or portion thereof), which should be paid directly to the Copyright Clearance Center (CCC), 222 Rosewood Drive, Danvers, MA 01923. Payment may also be made electronically through CCC Online at copyright.com. Other copying for republication, resale, advertising or promotion, or any form of systematic or multiple reproduction of any material in this book is prohibited except with permission in writing from the publisher. The CCC fee code is 0277-786X/08/\$18.00.

Printed in the United States of America.

Publication of record for individual papers is online in the SPIE Digital Library.

SPIE 
Digital Library

SPIDigitalLibrary.org

Paper Numbering: Proceedings of SPIE follow an e-First publication model, with papers published first online and then in print and on CD-ROM. Papers are published as they are submitted and meet publication criteria. A unique, consistent, permanent citation identifier (CID) number is assigned to each article at the time of the first publication. Utilization of CIDs allows articles to be fully citable as soon they are published online, and connects the same identifier to all online, print, and electronic versions of the publication. SPIE uses a six-digit CID article numbering system in which:

- The first four digits correspond to the SPIE volume number.
- The last two digits indicate publication order within the volume using a Base 36 numbering system employing both numerals and letters. These two-number sets start with 00, 01, 02, 03, 04, 05, 06, 07, 08, 09, 0A, 0B ... 0Z, followed by 10-1Z, 20-2Z, etc.

The CID number appears on each page of the manuscript. The complete citation is used on the first page, and an abbreviated version on subsequent pages. Numbers in the index correspond to the last two digits of the six-digit CID number.

Contents

- vii *Conference Committee*
- ix *Introduction*
- xi *Measurement science for climate remote sensing (Plenary Paper) [7081-53]*
G. T. Fraser, S. W. Brown, R. U. Datta, B. C. Johnson, K. R. Lykke, J. P. Rice, National Institute of Standards and Technology (United States)

SESSION 1 SYSTEM MODELING AND SIMULATION

- 7087 03 **PICASSO: an end-to-end image simulation tool for space and airborne imaging systems** [7087-02]
S. A. Cota, J. T. Bell, R. H. Boucher, T. E. Dutton, C. J. Florio, G. A. Franz, T. J. Grycewicz, L. S. Kalman, R. A. Keller, T. S. Lomheim, D. B. Paulson, T. S. Wilkinson, The Aerospace Corp. (United States)
- 7087 04 **Focal plane resolution and overlapped array TDI imaging** [7087-03]
T. J. Grycewicz, S. A. Cota, T. S. Lomheim, L. S. Kalman, The Aerospace Corp. (United States)
- 7087 05 **Noise equivalent reflectance difference (NERD) vs. spatial resolution (SR) as a good measure for system performances** [7087-05]
M. Citroen, G. Raz, M. Berger, Elbit Systems, Electro-Optics El-Op, Ltd. (Israel)
- 7087 06 **Simulation of Meteosat Third Generation-Lightning Imager through tropical rainfall measuring mission: Lightning Imaging Sensor data** [7087-06]
D. Biron, L. De Leonibus, Ctr. Nazionale di Meteorologia e Climatologia Aeronautica (Italy); P. Laquale, D. Labate, Selex Galileo (Italy); F. Zauli, D. Melfi, Ctr. Nazionale di Meteorologia e Climatologia Aeronautica (Italy)

SESSION 2 GEOPHYSICAL PRODUCT SYSTEMS ENGINEERING

- 7087 07 **Application of OSSEs to observing system design** [7087-07]
R. Atlas, National Oceanic and Atmospheric Administration (United States); L. P. Riishojgaard, Joint Ctr. for Satellite Data Assimilation, NOAA Science Ctr. (United States)
- 7087 08 **Image quality vs. sensitivity: fundamental sensor system engineering** [7087-08]
C. F. Schueler, Orbital Sciences Corp. (United States)
- 7087 09 **Zombie algorithms: a timesaving remote sensing systems engineering tool** [7087-09]
P. E. Ardanuy, Raytheon Information Solutions (United States); D. C. Powell, Lockheed Martin Corp. (United States); S. Marley, Raytheon Intelligence and Information Systems (United States)

- 7087 0B **Application of satellite surface wind data to ocean wind analysis** [7087-11]
R. Atlas, National Oceanic and Atmospheric Administration (United States); J. Ardizzone, NASA Goddard Space Flight Ctr. (United States); R. N. Hoffman, Atmospheric and Environmental Research, Inc. (United States)

SESSION 3 GEOPHYSICAL PRODUCT SYSTEMS ENGINEERING II

- 7087 0C **Geospatial visualization of atmospheric chemistry satellite data using Google Earth** [7087-12]
J. Burke, Raytheon Intelligence and Information Systems (United States)
- 7087 0F **Near real time data processing system** [7087-15]
A. Mousessian, C. Vuu, Raytheon Intelligence and Information Systems (United States)

SESSION 4 SENSOR SYSTEMS ENGINEERING AND TECHNOLOGY

- 7087 0G **System engineering studies for advanced geosynchronous remote sensors: some initial thoughts on the 4th generation** [7087-16]
J. J. Puschell, L. Cook, Y. J. Shaham, M. D. Makowski, J. F. Silny, Raytheon Space and Airborne Systems (United States)
- 7087 0H **Jitter suppression techniques for mechanical cryocooler-induced disturbances** [7087-18]
D. W. Wolfe, C. S. Kirkconnell, G. L. Fleischman, W. H. Sunada, Raytheon Space and Airborne Systems (United States)
- 7087 0I **Real-time simultaneous temperature and strain measurements at cryogenic temperatures in an optical fiber** [7087-19]
S. Mahar, Massachusetts Institute of Technology (United States); J. Geng, NP Photonics (United States); J. Schultz, J. Minervini, Massachusetts Institute of Technology (United States); S. Jiang, NP Photonics (United States); P. Titus, M. Takayasu, C. Gung, Massachusetts Institute of Technology (United States); W. Tian, A. Chavez-Pirson, NP Photonics (United States)
- 7087 0J **Design of the stereoscopic eye-tracking system for quantitative remote sensing applications** [7087-20]
A. Sergeyev, E. Levin, M. C. Roggemann, Michigan Technological Univ. (United States); G. Gienko, The Univ. of the South Pacific (Fiji)
- 7087 0M **One-dimensional tomographic fiber-optic measuring system based upon single fiber multimode interferometers** [7087-23]
A. D. Lantsov, Far Eastern State Technical Univ. (Russia); O. B. Vitrik, Y. N. Kul'chin, Institute for Automation and Control Processes (Russia)

SESSION 5 COMMERCIAL ASSETS IN FUTURE REMOTE SENSING SYSTEMS

- 7087 0N **Iridium NEXT partnership for Earth observation: exploiting global satellite constellations for new remote sensing capabilities** [7087-24]
O. P. Gupta, Iridium Satellite LLC (United States)

- 7087 0O **Use of commercial assets in future remote sensing systems** [7087-25]
G. Jansson, Intelsat Global Corp. (United States)
- 7087 0P **The Boreas concept for imaging polar winds from the Iridium-NEXT constellation** [7087-26]
D. Chesters, NASA Goddard Space Flight Ctr. (United States); L. P. Riishojgaard, Joint Ctr.
for Satellite Data Assimilation (United States)
- 7087 0Q **Commercial solution for ocean color: SeaWiFS-2 rideshare with GeoEye-2** [7087-27]
M. G. Hammann, GeoEye, Inc. (United States); J. J. Puschell, C. Schueler, Raytheon Space
and Airborne Systems (United States)
- 7087 0R **A standardized interface and accommodation methodology for commercially hosted
payloads on the StarBus** [7087-28]
P. C. Kalmanson, C. Schueler, M. Do, Q. Lam, Orbital Sciences Corp. (United States)

Author Index

Conference Committee

Program Track Chair

Allen H. L. Huang, University of Wisconsin, Madison (United States)

Conference Chairs

Philip E. Ardanuy, Raytheon Intelligence and Information Systems
(United States)

Jeffery J. Puschell, Raytheon Space and Airborne Systems
(United States)

Cochairs

Hal J. Bloom, NOAA, GOES-R Program (United States)

Allen H. L. Huang, University of Wisconsin, Madison (United States)

Program Committee

Stephen A. Cota, The Aerospace Corporation (United States)

William B. Gail, Microsoft Corporation (United States)

Gerry Jansson, Intelsat Global Service Corporation (United States)

Jay Pearlman, The Boeing Company (United States)

Lars-Peter Riishojgaard, Joint Center for Data Assimilation
(United States)

Donald L. Thoma, Iridium Satellite LLC (United States)

Session Chairs

- 1 System Modeling and Simulation
Jeffery J. Puschell, Raytheon Space and Airborne Systems
(United States)
- 2 Geophysical Product Systems Engineering
Philip E. Ardanuy, Raytheon Intelligence and Information Systems
(United States)
- 3 Geophysical Product Systems Engineering II
Philip E. Ardanuy, Raytheon Intelligence and Information Systems
(United States)

- 4 Sensor Systems Engineering and Technology
Jeffery J. Puschell, Raytheon Space and Airborne Systems
(United States)
- 5 Commercial Assets in Future Remote Sensing Systems
Jeffery J. Puschell, Raytheon Space and Airborne Systems
(United States)

Introduction

This volume contains the proceedings from the first SPIE conference on Remote Sensing System Engineering. The conference was held 11–13 August 2008 in San Diego, California, as part of the Optical Engineering + Applications section of SPIE Optics + Photonics.

The goals of this conference were to discuss existing and emerging design approaches, engineering methods, tools, and future trends for engineering of remote sensing systems. This topic included: (1) system architecture and design, (2) requirements, performance metrics and measures of success, (3) modeling and simulation tools and methods, (4) design and integration of distributed architectures, (5) use of commercial assets in future remote sensing systems, and (6) the end user, effective data/information/system utilization, and optimum return on investment.

To achieve these goals, papers were solicited in, but not limited to, the following areas:

- system architecture and design for current and future experimental, research, and operational Earth and space remote sensing programs and experiments
- system engineering metrics and measures of success leading to optimal system design
- methods and approaches for system requirements identification, definition and allocation for operational programs and experiments
- end-to-end system modeling and simulation methods and tools
- system engineering approaches for optimizing transition of research systems to operational use
- distributed remote sensing system architectures
- evolution of systems to networks
- integrated system of systems: engineering approaches and methods
- remote sensors as secondary payloads onboard satellite communication systems such as Intelsat and Iridium NEXT
- use of commercial visualization software such as Google Earth and Microsoft Virtual Earth in remote sensing systems.

A total of 25 papers were presented in five sessions. We enjoyed the participation of a diverse group of international researchers from government, academia, and industry. The range of topics was remarkable and included system modeling and simulation, geophysical product system engineering, sensor systems engineering and technology, and use of commercial assets in future remote sensing systems.

We thank all of the participants who made this conference successful, especially the cochairs, program committee, and authors.

Philip E. Ardanuy
Jeffery J. Puschell

Measurement science for climate remote sensing

G. T. Fraser, S.W. Brown, R.U. Datla, B.C. Johnson, K.R. Lykke, J.P. Rice
Optical Technology Division, National Institute of Standards and Technology
Gaithersburg, MD 20899-8440

ABSTRACT

The NIST role in supporting our Nation's climate research is described. The assembly of climate data records over decadal time scales requires assimilating readings from a large number of optical sensors deployed in space and on the Earth by various nations. NIST, in partnership with NASA and NOAA, develops and disseminates the calibration tools and standards to ensure that the measurements from these sensors are accurate, comparable, and tied to international standards based on the SI system of units. This effort helps to provide confidence that the small decadal changes in environmental variables attributed to climate change are not an artifact of the measurement system. Additionally, it ensures that the measurements are physics based and thus comparable to climate models.

Keywords: climate change, measurement science, metrology, remote sensing

1. INTRODUCTION

The Earth's climate is complex and highly variable, making it difficult to measure and model small changes that occur over decadal and longer time scales. The resulting uncertainties in measurement and modeling underlie the long-term debate over the direction, magnitude, and consequence of climate change.

Even as the consensus grows on climate change, climate monitoring will continue to be necessary to quantify regional variation; to establish the effectiveness of mitigation efforts, including possible geo-engineering solutions;¹ and to address the potential for catastrophic climate change events not easily amendable to modeling. Also, climate monitoring, as demonstrated in the past, is critical for the detection and mitigation of other anthropogenic environmental problems unrelated to greenhouse gas releases, such as the depletion of the Earth's stratospheric ozone layer by chlorofluorocarbons and possible future global warming from anthropogenic heat release.²

This paper focuses on the measurement challenges associated with monitoring the Earth's climate. The discussion emphasizes the passive measurement of electromagnetic radiation, which encompasses nearly all satellite measurements used in climate research. The viewpoint for the discussion is from the field of metrology, the science of measurement.

Of particular interest here are measurements required to create environmental data records, for example, global mean surface temperature as a function of time. Such long-term measurements generally have higher accuracy requirements than short-term measurements taken to quantify a specific phenomenology related to climate for use in initializing or advancing climate models.

A short-term measurement strategy emphasizing the characterization of phenomenology in the absence of supporting long-term measurement strategy to create environmental data records leads to the requirement that climate models provide the direction and magnitude of changes in climate variables. Such short-term measurements targeting specific phenomenology often do not meet the accuracy requirements or measurement time interval for creating long-term data records to monitor and track climate change. A long-term measurement strategy relies on developing highly accurate data records for specific climate variables to establish trends. Such a strategy requires sustaining high-quality measurements over decadal time scales to ascertain trends.

The need to have "immediate" answers to climate questions has led to efforts to use data records from instruments initially intended for weather forecasting and other applications having less stringent measurement uncertainty requirements than climate. An example of such an effort is the application of microwave sounding measurements from National Oceanic and Atmospheric Administration (NOAA) polar-orbiting weather satellites to detect trends in atmospheric temperature for comparison against climate modeling predictions.³ The retrospective analysis of such inherently "lower" quality measurements to improve their quality necessarily leads to increased subjectivity in the

analysis. Such an analysis is subject to present expectations for the magnitude and direction of change in the climate variable of interest which has the potential to bias the analysis. The continued debate over the microwave sounding measurements illustrates the inherent controversy in this approach.^{4,5} Only top-of-the-atmosphere solar irradiance has had a long-term satellite effort for monitoring that approaches the level of accuracy required for climate research.⁶

2. CLIMATE MEASUREMENT REQUIREMENTS

Although the potential for climate change first came to the forefront from evidence of increasing atmospheric carbon dioxide obtained from chemical measurements on air samples acquired on Mauna Loa, Hawaii,⁷ at a fundamental physics level, monitoring the Earth's climate reduces to a problem in the measurement of electromagnetic radiation. As illustrated in Figure 1, at equilibrium, the incoming solar radiation, $\pi R_{Earth}^2 S_{Earth}$, balances the reflected solar radiation, $\pi R_{Earth}^2 \rho_{Earth} S_{Earth}$, and the emitted thermal infrared radiation, $4\pi R_{Earth}^2 \sigma \epsilon_{Earth} T_{Earth}^4$. Any long-term change in the solar constant, (S_{Earth}), in the Earth's globally averaged reflectivity (i.e., albedo) (ρ_{Earth}), or in the Earth's globally averaged emissivity (ϵ_{Earth}) will lead to a change in the Earth's globally averaged temperature, T_{Earth} , with the rate of change dependent on an effective time constant which encompasses a variety of phenomena such as vertical thermal transport within the oceans.

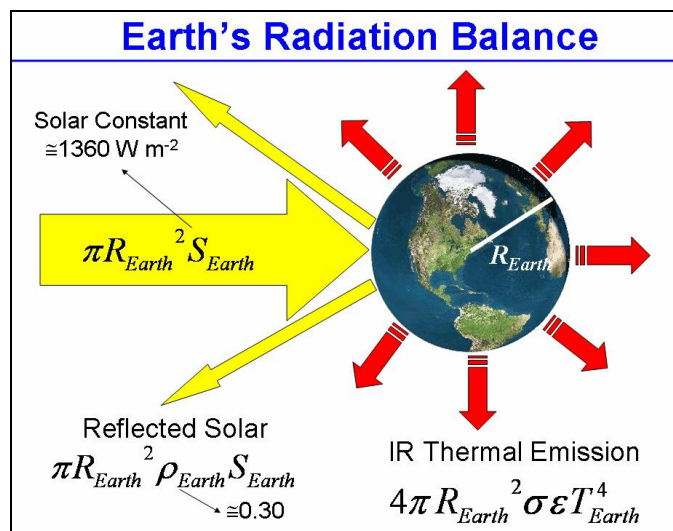


Fig. 1. A simple picture for the Earth's radiation balance. Here, ρ_{Earth} is the albedo of the Earth, σ is the Stefan-Boltzmann constant, T_{Earth} is the global mean temperature of the Earth, R_{Earth} is the radius of the Earth, S_{Earth} is the solar irradiance at the top of the atmosphere, IR is infrared, and ϵ_{Earth} is the global mean emissivity of the Earth.

The sensitivity of the Earth's temperature to small changes in S_{Earth} , ρ_{Earth} , and ϵ_{Earth} provides estimates for the measurement accuracy requirements for these three parameters for their use in climate research. Changes in S_{Earth} are natural in origin, whereas changes in ρ_{Earth} , and ϵ_{Earth} have anthropogenic contributions; greenhouse gases and black aerosols for ϵ_{Earth} , and sulfate aerosols and changes in land use for ρ_{Earth} .

As an example, consider the changes in solar irradiance, globally averaged albedo, and globally averaged emissivity required to cause an increase in the Earth's mean temperature of 1 K/100 yrs or 0.01 K/yr, approximately the current rate of global warming over the last century. A 0.01K/yr increase in global mean temperature corresponds to a 0.19 Wm^{-2}/yr (0.014 %/yr) increase in solar irradiance, a 0.033 %/yr decrease in albedo, or a 0.015 %/yr decrease in emissivity.

These numbers can be compared with the uncertainties in radiometric standards disseminated by NIST which generally fail to meet the stringent requirements for climate monitoring by an order of magnitude or more:

- Spectral irradiance lamp standards for the wavelength range of 250 nm to 2400 nm have uncertainties of 0.3 % to 1.6 % ($k = 2$ or 2σ), depending on wavelength.
- Pressed and sintered polytetrafluoroethylene (PTFE) reflectance standards for near-normal incident directional hemispherical reflectance have uncertainties varying from 0.67 % at 200 nm to 0.21 % at 1600 nm.

- Spectral emissivity standards from 1 μm to 14 μm have uncertainties of approximately 1 % for a Lambertian material with $\varepsilon \approx 0.6$.

Programs needing lower uncertainties must work directly with NIST to have direct access to laboratory calibration tools such as the Primary Optical Watt Radiometer (POWR) and the Facility for Spectral Irradiance and Radiance Responsivity Calibrations using Uniform Sources (SIRCUS) discussed below, however, even these capabilities are generally not sufficient to enable remote-sensing instruments to achieve the low uncertainties required for detecting and monitoring small changes in the Earth's radiation balance expected with climate change.

Measuring small changes in radiometric sources at the level of uncertainty required for climate monitoring is extremely challenging, be it the Earth, Sun, or a laboratory source or artifact. That no validated satellite remote-sensing instrument has achieved the uncertainty requirements for monitoring any of the three components (solar, reflected solar, or emitted infrared) of the Earth's radiative balance attests to the challenge. Moreover, the measurement uncertainties for climate quoted above are even more stringent (by approximately a factor of 3 ignoring correlation) if a combination of changes in solar irradiance, albedo, and emissivity are considered. In realization of this measurement challenge scientists have resorted to the tracking of secondary environmental variables, such as sea-ice extent in the Arctic, which are more sensitive to climate change but also more difficult to include in climate models.

Adding to the measurement challenge is that changes in the Earth's climate system must be detected against the larger natural fluctuations that arise from day-to-day weather variations, the seasons, the eleven-year solar cycle, and major cyclical climate phenomena such as El Niño and La Niña. Despite such fluctuations, the reliability of climate trending from environmental data records continues to benefit from reductions in measurement uncertainty.⁸

Further details on measurement requirements for climate are provided in the report of a 2002 workshop cosponsored by NIST, NASA, NOAA, and NPOESS/NPP (National Polar-orbiting Operational Environmental Satellite System/NPOESS Preparatory Project). The report emphasizes satellite-based measurements.⁹ A follow-on report recently released addresses strategies to reach these requirements.¹⁰

3. NEED FOR TRACEABILITY TO SI STANDARDS WITH LOW UNCERTAINTIES TO MEET CLIMATE REQUIREMENTS

The ability to unambiguously detect and accurately quantify small yearly changes in the Earth's climate over decadal and longer time scales requires that the measurements be tied, i.e., traceable, to international standards based on the International System of Units, the SI, as maintained by national metrology institutes such as NIST. This viewpoint has been articulated in the Strategic Plan for the U.S. Climate Change Program¹¹ and in an agreement¹² between the World Meteorology Organization (WMO), representing national weather services, and the International Committee for Weights and Measures (CIPM), representing national measurement laboratories.

SI traceability has several advantages for climate research. It ensures that the measurements are based on the fundamental laws of physics and thus can be compared with predictions from physics-based modeling. Physics-based modeling is critical for developing climate models that are objective and have the flexibility to advance as the state of knowledge of climate physics improves and computational capabilities increase.

SI traceability also allows measurements to be compared independent of time or of the organization or country performing the measurements. Measurement comparability is essential for the success of international efforts dependent on exchange and integration of measurements, such as the Global Earth Observation System of Systems (GEOSS).¹³

Except for the kilogram, the ability to realize a standard for an SI unit does not require access to a specific artifact. Thus, SI-based standards can be and are realized and disseminated by NIST and other National Measurement Institutes (NMIs) around the world without access to specific artifacts. The standards and any changes in the standards are well documented by the NMIs, providing the necessary information to tie past and future realizations of the SI units with present realizations. Additionally, the NMIs validate and document the quality of their SI standards through measurement comparisons held under the auspices of the International Committee for Weights and Measures formed by the Treaty of the Meter. The results from such comparisons are made available on the website of the Bureau of Weights and Measures (BIPM).¹⁴

The results from one such measurement comparison relevant to climate research is shown in Figure 2.¹⁵ The Figure illustrates the level of agreement with respect to a reference value for measurements of the spectral irradiance of 1 kW FEL-type quartz-tungsten-halogen lamps by 12 participating national metrology institutes, including NIST.

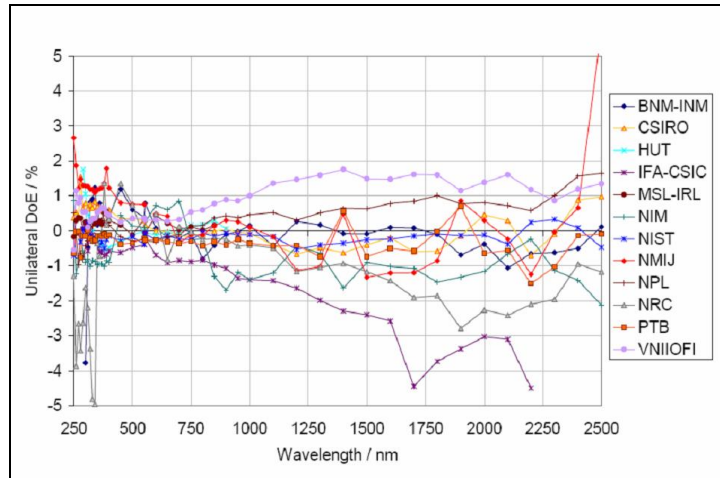


Fig. 2. Results from an international comparison of spectral irradiance measurements between National Metrology Laboratories (NMIs). Measurements are given as a percent difference relative to a reference value. The acronyms reference the twelve participating NMIs and are defined at http://www.bipm.org/en/practical_info/acronyms.html.

These lamps are typically used by remote-sensing scientists to realize a spectral radiance scale by illuminating a near-perfect Lambertian reflector consisting of pressed and sintered polytetrafluoroethylene. The measurement mimics in the laboratory the illumination of the Earth by the Sun, although the color temperature of the lamp of 2950 K is approximately a factor of two smaller than the approximately 5900 K radiance temperature of the Sun as measured at the top of the atmosphere. This discrepancy between the spectral outputs of the FEL lamp and the Sun needs to be addressed in calibrating instruments monitoring direct or reflected solar radiation to reduce spectrally dependent stray light errors. Note that the typical agreement of approximately 1 % in the intercomparison is approximately two orders of magnitude larger than the uncertainty requirement for long-term monitoring of the total solar irradiance of the Sun.

4. NIST INFRARED-TO-ULTRAVIOLET SI RADIATION STANDARDS

NIST standards for the measurement of electromagnetic radiation from the infrared to the ultraviolet are tied to the watt, kelvin, and meter. An extensive infrastructure has been developed to ensure the ability of NIST to provide the lowest uncertainty standards for various applications in industry, defense, and environment. Climate research, in particular, requires standards with extremely low uncertainty to meet the stringent measurement requirements discussed above. The low uncertainty requirements for climate have provided the greatest drive for reducing the uncertainties in NIST’s fundamental and disseminated electromagnetic radiation standards.

The Primary Optical Watt Radiometer (POWR) is the NIST developed and maintained National standard for measurement of optical power.¹⁶ POWR shown in Figure 3 is a liquid-helium-cooled cryogenic radiometer which compares the optical power from a laser beam incident on a high-absorptivity optical cavity with the electrical power dissipated by a resistor in thermal contact with the cavity, thus tying the optical watt to the electrical watt. The laser beam of known optical power determined to an expanded relative uncertainty $k = 2$ of 0.02 % as verified through international comparisons among NMIs is used to calibrate extremely linear, high-dynamic-range silicon trap detectors for measurement of the radiance [$\text{W m}^{-2} \text{sr}^{-1}$] or irradiance [W m^{-2}] of integrating sphere sources used to calibrate remote sensing instruments. Trap detectors typically have a circular optical aperture of accurately known area with diameter larger than the laser beam diameter to realize an absolute irradiance responsibility standard, or absolute spectral irradiance responsivity standard if the laser wavelength is varied in the transfer of the calibration from POWR to the trap detector.

To measure the area of the apertures used in the realization of an irradiance or radiance standard a coordinate measurement machine (CMM) is used. The CMM uses an optical microscope to map the coordinates of the edges of the aperture as it is moved through the focus of the microscope.¹⁷ The relative position of the x-y translation stage used in

the mapping of the aperture is measured interferometrically by referencing to etalon fringes generated from a frequency stabilized HeNe. The laser interferometry ties the aperture area determination to the meter through the accurately known wavelength of the HeNe laser. The resulting aperture-area measurements have uncertainties of less than 0.01 % $k = 2$. The uncertainties have been validated through international comparisons which also revealed significant discrepancies below the 0.01 % level between aperture measurements performed using optical methods and contact methods.¹⁸

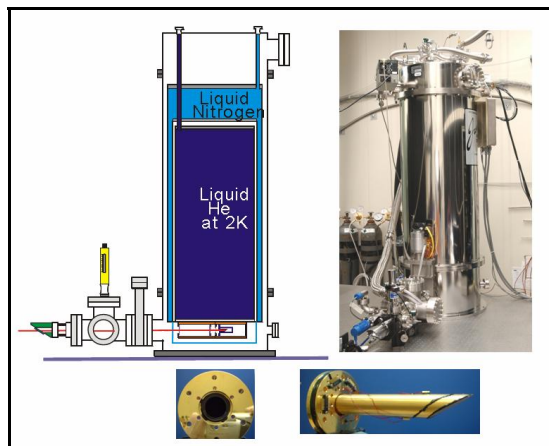


Fig. 3. A schematic diagram and picture of the NIST Primary Optical Watt Radiometer (POWR), the Nation’s primary standard for optical power. POWR is a cryogenic radiometer which compares optical power to electric power to tie the optical watt to the electrical watt. POWR can determine the optical power in a laser beam to 0.02 % $k = 2$.

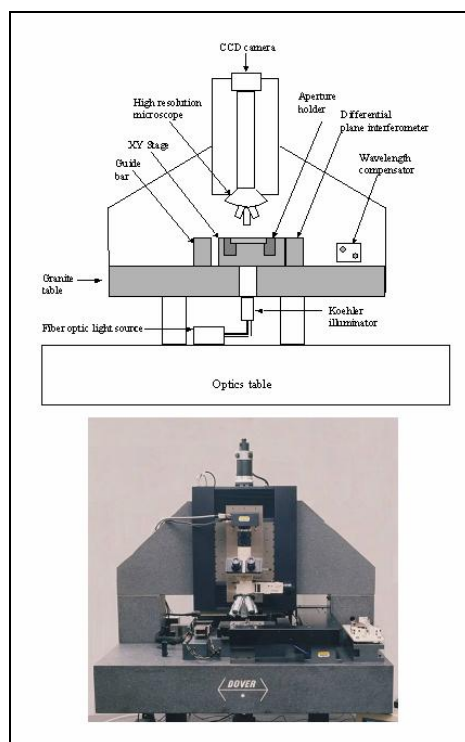


Fig. 4. A schematic diagram and picture of the NIST Absolute Aperture Area Measurement Facility. The facility uses an optical microscope to view the edge points of an optical aperture as it is moved through the focus of the microscope on an interferometrically controlled x-y translation stage. The area of an aperture is determined to better than 0.01 % ($k = 2$).

Use of apertures in irradiance or radiance standards requires correction for diffraction effects, particularly for long wavelengths and small apertures, or when the measurement requirements are particularly stringent. NIST has developed sophisticated models to correct for diffraction effects in radiometry. Diffraction corrections have played a critical role in a number of applications, including satellite measurements of solar irradiance,¹⁹ infrared photometric measurements of stars,²⁰ and infrared measurements of blackbodies in low-thermal-background space vacuum chambers used in testing sensors for ballistic missile defense.²¹

To transfer the radiometric scales achieved above to various sensors used in climate research, NIST has developed a unique laser-based facility called SIRCUS for Spectral Irradiance and Radiance Responsivity Calibrations using Uniform Sources.²² SIRCUS uses a set of wavelength-tunable lasers from the infrared to the ultraviolet fiber-coupled to the interior of an integrating sphere with an exit port to provide a source of known radiance or irradiance as defined through an appropriate set of apertures and referenced absolutely using a trap detector. SIRCUS allows the absolute calibration of optical radiation sensors to approximately 0.05 % in spectral responsivity provided that the sensor is sufficiently stable to hold the calibration through the time it is used. Additionally, SIRCUS provides an end-to-end system level calibration of the sensor under real illumination conditions that fully fill the entrance pupil to the sensor.

At longer wavelengths, i.e., in the thermal infrared, NIST's room-temperature-background radiometric scales are based on high-emissivity blackbody sources with radiance levels tied to the kelvin through contact thermometry. One such blackbody is the so-called NIST Water Bath Blackbody (WBBB) based on a black-painted 10.8 cm diameter, 25 cm deep, conical optical cavity immersed in a reservoir of water whose temperature is variable over the range 15 °C to 80 °C and measured using accurate platinum resistance thermometers. The WBBB was used to validate the radiometric scales of several programs involved in the measurement of sea-surface temperature (SST).²³

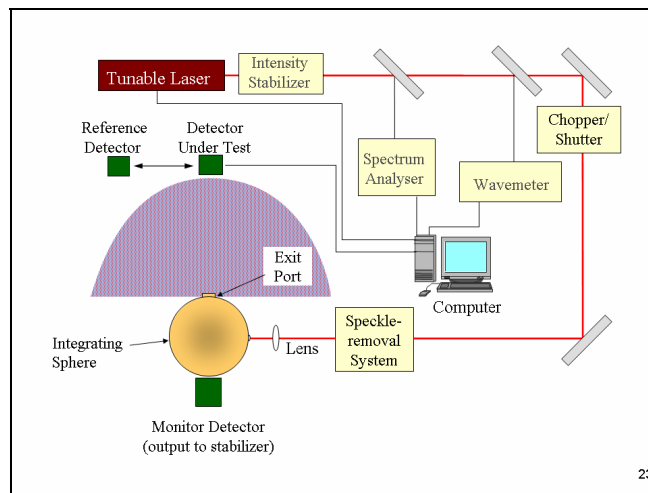


Fig. 5. A schematic diagram and picture of the NIST Facility for Spectral Irradiance and Radiance Responsivity Calibrations using Uniform Sources (SIRCUS). SIRCUS uses a suite of lasers from the short wavelength infrared (SWIR) to the ultraviolet (UV) to illuminate an integrating sphere source to produce a uniform radiance source of known absolute intensity as determined using standard trap detectors calibrated against a cryogenic radiometer such as POWR.

5. EXTENDING TRACEABILITY WITH LOW UNCERTAINTES TO CLIMATE MEASUREMENTS—PRELAUNCH CALIBRATION

Satellite programs generally have requirements that the prelaunch radiometric calibration be tied to international standards based on the SI system of units. One of the twenty Global Climate Observing System (GCOS) Climate Monitoring Principles²⁴ affirm this goal by stating, “Rigorous pre-launch instrument characterization and calibration, including radiance confirmation against an international radiance scale provided by a national metrology institute, should be ensured.” Ground-based measurements likewise need such traceability to help validate and calibrate satellite measurements and ensure comparability with satellite measurements when integrated into climate data records. In response to these needs NIST has developed a variety of standards, calibration tools, and training resources to help establish the traceability of climate measurements to the SI system of units.

For near-infrared to ultraviolet radiation standards, NIST provides calibration services for spectral radiance standards based on lamp-illuminated integrating spheres, spectral reflectance standards based on polytetrafluoroethylene, and spectral-irradiance standards based on FEL lamps. The latter two standards when used together provide a spectral radiance standard. The polytetrafluoroethylene plaque is illuminated at normal incidence with a known spectral irradiance level from the FEL lamp producing a spectral radiance standard when viewed, typically at 45° off normal as the plaque reflectance is usually measured for this so-called 0°/45° geometry. A typical user of integrating sphere and lamp-plaque radiance standards achieves agreement with the NIST radiance scale to approximately 2 %, as demonstrated by a recent spectral radiance scale intercomparison between 10 laboratories involved in ocean color research.²⁵ Similarly, a 2 % agreement is also seen when comparing bidirectional reflectance distribution function (BRDF) measurements on polytetrafluoroethylene reflectance standards.²⁶

In collaboration with the Earth Observing System (EOS) satellite program, NIST has developed a series of standard radiometers and radiance standards to validate the radiometric scales of the satellite programs. These radiometers have been well described in the literature and include the Thermal-infrared Transfer Radiometer (TXR), a mid-wave and long-wave thermal-infrared radiometer; the six-channel filter-based Visible Transfer Radiometer (VXR); and the Short-Wave Infrared Radiometer (SWXIR). The VXR has been used to verify the visible and near-infrared radiance scales of the lamp-illuminated integrating spheres used in support of the Moderate Resolution Imaging Spectrometer (MODIS), the Multi-angle Imaging Spectrometer (MISR), and the Advanced Spaceborne Thermal Emission and Reflection Radiometer (ASTER) while the SWXIR has been used to validate the short-wave infrared radiance scale of the MODIS sphere. The TXR has supported the Multispectral Thermal Imager (MTI),²⁷ Geostationary Operational Environmental Satellite (GOES) imager, Moderate Resolution Imaging Spectroradiometer (MODIS), and the NPOESS Visible Infrared Imaging Spectroradiometer Suite (VIIRS) and Cross-track Infrared Sounder (CRIS).

NIST has also developed a version of SIRCUS, denoted Traveling SIRCUS, designed for transportation to satellite and ground-sensor test and evaluation facilities to perform full system-level characterization and calibration of sensors operating from the near-infrared to the ultraviolet, within the reflected solar region. Traveling SIRCUS has been used to calibrate and characterize the Earth Polychromatic Imaging Camera (EPIC), the Marine Optical Buoy (MOBY), and the Robotic Lunar Observatory (ROLO), as well as several astronomical telescope systems.

6. EXTENDING TRACEABILITY WITH LOW UNCERTAINTIES TO CLIMATE MEASUREMENTS—POST-LAUNCH CALIBRATION

The challenge remains to verify that the prelaunch calibration is maintained on orbit. On-orbit SI traceability mitigates the risk associated with a satellite failure in the creation of long-term data records. A number of strategies have been developed to assess, maintain, and improve the quality of satellite measurements on orbit, including using so called vicarious calibration sites based on Earth targets such as deep convective clouds and desert scenes, the Moon, or stars; satellite measurement comparisons; and on-board calibration.

In the event of continuous monitoring of one or more climate variables using a series of satellites, such as the NOAA geostationary and polar-orbiting satellites, data records have been generated using the strategy as outlined in Figure 6. Here the individual measurement time series or data records are merged into one continuous record by choosing one of the satellites as the reference and using the satellite measurement temporal overlaps to align all the other satellite measurements to the reference satellite measurements. The satellite overlaps could be averaged over some portion of the overlap period, such as done with top-of-the-atmosphere solar irradiance measurements, or could be based on simultaneous measurements using actual spatial and temporal overlaps, so called Simultaneous Nadir Overlaps (SNOs),²⁸ which occur most often in the polar regions for polar-orbiting satellites. A difficult to test assumption in generating such lengthy time series is that the satellites do not share any systematic instrument drift. This assumption may not always hold at the level required for climate research as typically satellite instruments involved in the creation of such long time series share significant hardware and calibration heritage and thus are potentially prone to common systematic drifts.

The Moon and stars are also used to provide a relative calibration of satellite sensors and to track sensor degradation. The lack of a Lunar atmosphere, the absence of significant geological activity, and constant solar exposure over billions of years provide confidence in the assumption that the surface reflectance is constant over the decadal time scales

associated with satellite remote sensing of the Earth’s climate. Using Earth-viewing sensors to view the Moon in combination with the Lunar reflectance model developed by the Robotic Lunar Observatory (ROLO)²⁹ to correct for the effect of the Moon’s phase and libration on the satellite measurement has been demonstrated to be an effective approach for long-term tracking of instrument stability within a spectral channel.³⁰ A concept has been proposed called LUSI for Lunar Spectral Irradiance³¹ for improving the absolute calibration of the Moon beyond the level achieved by ROLO.

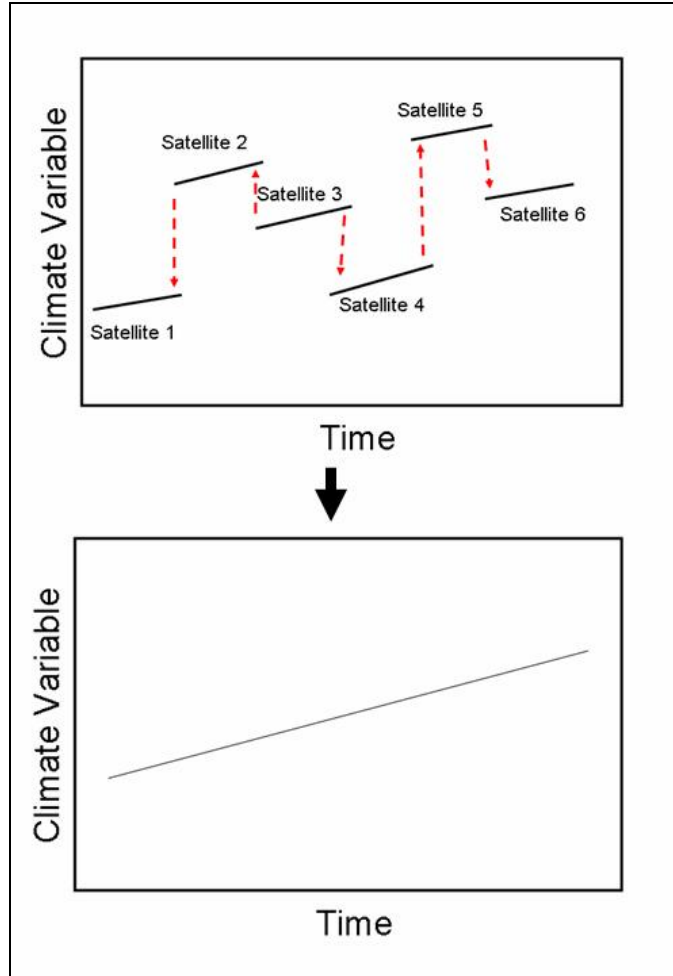


Fig. 6. The two panels demonstrate the creation of an environmental data record by stringing together a set of records from a series of satellites and shifting the individual satellite calibrations relative to one of the satellites taken as the standard or reference. This approach does not consider the possibility of shared drift among the satellites originating from their common heritage.

7. ESTABLISHING AND VALIDATING SI TRACEABILITY IN SPACE WITH LOW UNCERTAINTIES

One of the twenty Global Climate Observing System (GCOS) Climate Monitoring Principles states that “On-board calibration adequate for climate system observations should be ensured and associated instrument characteristics monitored.” Satellite programs continue to struggle with meeting this principle even though it is less stringent than the GCOS prelaunch principle referenced above advocating for “Rigorous pre-launch instrument characterization and calibration...” On-board calibration approaches include polytetrafluoroethylene reflectance standards which degrade in reflectivity from high-energy radiation and particles³² and have suffered from stray-light contamination due to earth shine.³³

Increased attention is being given to on-board satellite calibration. The need for improved space-based benchmark measurements of top-of-the-atmosphere spectral radiance emitted by the Earth has led to calls within the Decadal Survey³⁴ performed by the National Research Council for a CLARREO (Climate Absolute Radiance and Refractivity Observatory) mission in which the on-board sensor calibration to the SI system of units is rigorous. In principle, such benchmark instruments with appropriate spectral and spatial corrections could be used to calibrate other satellite instruments in support of the World Meteorological Organizations (WMO) Global Space-Based Inter-Calibration System (GSICS) effort.³⁵

8. THE NEED FOR LOWER UNCERTAINTY SI STANDARDS

Achieving the measurement requirements for long-term monitoring of the radiative balance of the Earth as illustrated in Figure 1 is challenging. Past and future efforts at meeting satellite measurement requirements in the context of the Earth Observing System experience have been discussed by Butler *et al.*³⁶ Remote-sensing programs using NIST-disseminated standards presently achieve radiometric uncertainties approximately two orders of magnitude larger than required for quantifying the radiative balance. Moreover, the uncertainties on the standards are also too large, by about an order of magnitude relative to the measurement requirements. The measurement requirements for monitoring the Earth's radiative balance have reached the limit of what can presently be achieved from the fundamental SI radiometric standards maintained at NIST. Research advances are required in all areas of the measurement traceability chain, from the fundamental standards to the disseminated standards to the remote sensing instrument calibration and characterization, to ensure that climate monitoring requirements are met.

SIRCUS and Traveling SIRCUS tied to cryogenic radiometry as discussed above are examples of tools that allow remote sensing programs to achieve instrument calibration at lower uncertainties relative to the SI than possible with standards typically disseminated by NIST such as spectral radiance standards based on a NIST calibrated integrating sphere source. NIST is also researching other approaches, including hyperspectral image projection³⁷, absolute pyrometry³⁸, spectrally tunable sources³⁹, and stray-light correction algorithms and characterization methods,⁴⁰ to improve the calibration of remote-sensing instruments tied to NIST standards. A long-term research program has also been implemented to develop alternative approaches for optical power standards based on the counting of individual photons as cryogenic radiometry has not advanced significantly over the last couple of decades beyond the 0.02% ($k = 2$) relative uncertainty level.

9. CONCLUSION

The accurate monitoring of the Earth's climate from using ground and space-based sensors will continue to depend on access to the highest accuracy fundamental SI standards for the passive measurement of electromagnetic radiation from the microwave to the ultraviolet spectral regions. Such standards are developed, maintained, improved, and compared by the world's National Metrology Institutes. Traceability to the SI ensures that measurements are comparable between organizations, countries, and over generations. Such traceability when established at a uncertainty level necessary to monitor the Earth's radiation balance provides confidence in the quality of climate data records used to predict the direction and rate of climate change. Additionally, SI traceable measurements are the foundation of climate models tied to the laws of physics.

ACKNOWLEDGMENTS

We would like to acknowledge our colleagues within the Optical Technology Division who have aided the effort to advance optical radiation standards to meet the demands for climate research.

REFERENCES

- [1] Such geo-engineering solutions include the controlled introduction of reflective sulfate aerosols into the upper atmosphere. See, for example, Crutzen, P. J., “Albedo Enhancement by Stratospheric Sulfur Injections,” *Climate Change* 77, 211–220 (2006).
- [2] Chaisson, E. J., “Long-Term Global Heating from Energy Usage,” *EOS* 89(28) (2008).
- [3] Karl, T. R., Hassol, S. J., Miller, C. D., and Murray, C. D. (editors), [Temperature Trends in the Lower Atmosphere: Steps for Understanding and Reconciling Differences], A Report by the Climate Change Science Program and the Subcommittee on Global Change Research, Washington, DC (2006).
- [4] See, for example, Randall, R. M. and Herman, B. M., “Using limited time period trends as a means to determine attribution of discrepancies in microwave sounding unit-derived tropospheric temperature time series,” *Journal of Geophysical Research-Atmospheres* 113(D5) D05105 (2008), and references therein.
- [5] See, for example, Zou, C. Z., Goldberg, M. D., Cheng, Z. H., Grody, N. C., Sullivan, J. T., Cao, C. Y., and Tarpley, D., “Recalibration of microwave sounding unit for climate studies using simultaneous nadir overpasses,” 111(D19), D19114 (2006), and references therein.
- [6] <http://spot.colorado.edu/~koppig/TSI>
- [7] Keeling, C. D., Bacastow, R. B., Bainbridge, A. E., Ekdahl, Jr., C. A., Guenther, P. R., Waterman, L. S., and Chin, J. F. S., “Atmospheric carbon dioxide variations at Mauna Loa Observatory, Hawaii,” *Tellus* 28, 538-551 (1976). Also see <http://www.esrl.noaa.gov/gmd/ccgg/trends/>.
- [8] Leroy, S. S., *et al.*, “Climate Signal Detection Times and Constraints on Climate Benchmark Accuracy Requirements,” *J. Climate*, to be published.
- [9] Ohring, G., Wielicki, B., Spencer, R., Emery, B., and Datla, R., (editors), [Satellite Instrument Calibration for Measuring Global Climate Change], Report of a Workshop Organized by National Institute of Standards and Technology (NIST), National Polar-orbiting Operational Environmental Satellite System-Integrated Program Office (NPOESS-IPO), National Oceanic and Space Administration (NOAA), National Aeronautics and Space Administration (NASA)], Workshop held at the University of Maryland Inn and Conference Center, College Park, MD, Nov. 12-14, 2002. Published as NISTIR 7047 (2004) available at <http://physics.nist.gov/Divisions/Div844/publications/NISTIR7047/nistir7047.pdf>.
- [10] Ohring, G. (editor), [Achieving Satellite Instrument Calibration for Climate Change (ASIC3)], Report of a Workshop Organized by National Oceanic and Atmospheric Administration, National Institute of Standards and Technology, National Aeronautics and Space Administration, National Polar-orbiting Operational Environmental Satellite System-Integrated Program Office, and Space Dynamics Laboratory of Utah State University at the National Conference Center, Lansdowne, VA, May 16-18, 2006. Available at <http://www.star.nesdis.noaa.gov/star/documents/ASIC3-071218-webversfinal.pdf>.
- [11] [Strategic Plan for the U.S. Climate Change Science Program], A Report by the Climate Change Science Program and the Subcommittee on Global Change Research (2003). Available at <http://www.climatechange.gov/Library/stratplan2003/final/ccspstratplan2003-all.pdf>.
- [12] “WMO and CIPM agree to consult together to ensure that data, related in particular to atmospheric composition and water resources, coming from the programmes of WMO are properly based on units traceable to the International System (SI) through the procedures of the Mutual Recognition Arrangement for National

Measurement Standards drawn up by the Committee and those of the Technical Regulations of WMO.” For further details see <http://www.bipm.org/utis/en/pdf/CIPM-WMO.pdf>.

- [13] See, for example, <http://www.epa.gov/geoss/>.
- [14] See www.bipm.org for further information.
- [15] Woolliams, E. R., Fox, N. P., Cox, M. G., Harris, P. M., and Harrison, N. J. "Final report on CCPR K1-a: Spectral irradiance from 250 nm to 2500 nm," Metrologia Technical Supplement 43, 02003 (2006). Also see http://kcdb.bipm.org/appendixB/KCDB_ApB_info.asp?cmp_idy=478&cmp_cod=CCPR-K1.a&prov=exalead.
- [16] Houston, J. M. and Rice, J. P., "NIST reference cryogenic radiometer designed for versatile performance," Metrologia 43 S31-35 (2006).
- [17] Fowler, J. and Litorja, M. "Geometric area measurements of circular apertures for radiometry at NIST," Metrologia 40(1), S9-S12 (2003).
- [18] Litorja, M., Fowler, J., Hartmann, J., Fox, N., Stock, M., Razet, A., Khlevnoy, B., Ikonen, E., Machacs, M., and Doytchinov, K., "Final report on the CCPR-S2 supplementary comparison of area measurements of apertures for radiometry," Metrologia Technical Supplement 44, 02002 (2007).
- [19] Butler, J. J., Johnson, B. C., Rice, J. P., Shirley, E. L., and Barnes, R. A., "Sources of differences in on-orbit total solar irradiance measurements and Description of a Proposed Laboratory Intercomparison," in press.
- [20] Witteborn, F. C., Cohen, M., Bregman, J. D., Wooden, D. H., Heere, K., and Shirley, E. L., "Spectral irradiance calibration in the infrared. XI. Comparison of alpha Bootis and 1 Ceres with a laboratory standard," Astronomical Journal 117(5), 2552-2560 (1999).
- [21] Carter, A. C., Datla, R. U., Jung, T. M., Smith, A. W., and Fedchak, J. A., "Low-background temperature calibration of infrared blackbodies," Metrologia 43 (2006) S46-S50.
- [22] Brown, S. W., Eppeldauer, G. P., and Lykke, K. R., "Facility for spectral irradiance and radiance responsivity calibrations using uniform sources," Applied Optics 45(32), 8218-8237 (2006).
- [23] Rice, J. P., Butler, J. J., Johnson, B. C., Minnett, P. J., Maillet, K. A., Nightingale, T. J., Hook, S. J., Abtahi, A., Donlon, C. J., and Barton, I. J., "The Miami 2001 infrared radiometer calibration and intercomparison: Part I. Laboratory characterization of blackbody sources," J. Atmos. and Oceanic Tech. 21(2), 258-267 (2004).
- [24] The Global Climate Observing System (GCOS) Climate Monitoring Principles are listed at <http://www.wmo.ch/pages/prog/gcos/index.php?name=monitoringprinciples>.
- [25] Meister, G., Abel, P., Carder, K., Chapin, A., Clark, D., Cooper, J., Davis, C., English, D., Fargion, G., Feinholz, M., Frouin, R., Hoge, F., Korwan, D., Lazin, G., McClain, C., McLean, S., Menzies, D., Poteau, A., Robertson, J., Sherman, J., Voss, K., and Yungel, J., The Second SIMBIOS Radiometric Intercomparison (SIMRIC-2), March – November 2002, NASA/TN-2002-210006, Vol. 2, Aug. 2003.
- [26] Early, E. A., Barnes, P. Y., and Johnson, B. C., Butler, J. J., Bruegge, C. J., Biggar, S. F., Spyak, P. R. and Pavlov, M. M., "Bidirectional Reflectance Round-Robin in Support of the Earth Observing System Program," Journal of Atmospheric and Oceanic Technology 17(8), 1077-1091 (2000).
- [27] Rice, J. P., Bender, S. C., Atkins, W. H., and Lovas, F. J., "Deployment test of the NIST EOS Thermal-infrared Transfer Radiometer," International Journal of Remote Sensing 24, 367-388 (2003).

- [28] Zou, C. -Z., Goldberg, M. D., Cheng, Z., Grody, N. C., Sullivan, J. T., Cao, C., and Tarpley, D. "Recalibration of microwave sounding unit for climate studies using simultaneous nadir overpasses," *Journal of Geophysical Research* 111, D19114 (2006).
- [29] T. C. Stone and H. H. Kieffer, "Use of the Moon to support on-orbit sensor calibration for climate change measurements," *Proc. SPIE* 6296 (2006). For additional references see <http://www.moon-cal.org/index.php>.
- [30] Eplee, Jr., R. E., Bailey, S. W., Barnes, R. A., Kieffer, H. H., and McClain, C. R., "Comparison of SeaWiFS On-Orbit Lunar and Vicarious Calibrations," *Proc. of SPIE* 6296, 629610 (2006).
- [31] Smith, A. W., Lorentz, S. R., Stone, T. C., Yoon, H., Datla, R. V., Pollock, D., and Tansock, J., "Lunar Spectral Irradiance and radiance (LUSI): Instrumentation to characterize the moon as an SI-traceable radiometric standard," http://www.goes-r.gov/downloads/GOES%20Users%20Conference%20V/GUC%20V%20Posters%202/poster_Smith%2021.pdf.
- [32] Xiong, X., Erives, H., Xiong, S., Xie, X., Esposito, J., Sun, J., Barnes, W., "Performance of Terra MODIS solar diffuser and solar diffuser stability monitor," *Proc. of SPIE* 5882, 58820S.1 (2005).
- [33] Wolfe, R. E., Esaias, W., Lyapustin, A., Xiong, X., "MODIS solar diffuser Earthshine modeling and analysis," *Proc. of SPIE* 6296, 629606 (2006).
- [34] [Earth Science and Applications from Space: National Imperatives for the Next Decade and Beyond], National Research Council, The National Academies Press (2007). Available at http://www.nap.edu/catalog.php?record_id=11820.
- [35] For further information visit the GSICS website at <http://www.star.nesdis.noaa.gov/smcd/spb/calibration/icvs/GSICS/index.html>.
- [36] Butler, J. J., Johnson, B. C., Rice, J. P., Brown, S. W., and Barnes, R. A., "Validation of radiometric standards for the laboratory calibration of reflected-solar Earth observing satellite instruments," *Proc. of SPIE* 6677, 667707 (2007).
- [37] Brown, S.W., Myers, B., Barnes, R. A., Rice, J. P., "Characterization of Earth observing satellite instruments for response to spectrally and spatially variable scenes," *Proc. of SPIE* 6677, 667705 (2007).
- [38] Allen, D. W., Saunders, R. D., Johnson, B. C., Gibson, C. E., and Yoon, H. W., "The Development and Characterization of an Absolute Pyrometer Calibrated for Radiance Responsivity," *AIP Conference Proceedings* 684, 577 (2003).
- [39] Fryc, I., Brown, S. W., Eppeldauer, G. P., and Ohno, Y., "LED-based spectrally tunable source for radiometric, photometric, and colorimetric applications," *Optical Engineering* 44(11), 111309 (2005).
- [40] Zong, Y., Brown, S. W., Johnson, B. C., Lykke, K. R., and Ohno, Y. "Simple spectral stray light correction method for array spectroradiometers," *Applied Optics* 45, 1111 (2006).